

DIESSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

## QUALITY CONTROL CERTIFICATE

KIT NAME DEAMIDATED GLIADIN-G - CHORUS

|         |         |
|---------|---------|
| Code    | 86100   |
| Lot No. | 879     |
|         | 2023-10 |
|         | 2022-10 |

## REAGENTS

| Label | Description                        | Lot. | Exp.    | NO  |
|-------|------------------------------------|------|---------|-----|
| D8660 | Deamidated Gliadin-G               | 879  | 2023-10 | 6X6 |
| B8660 | CALIBRATORE Deamidated Gliadin-G   | 879  | 2023-10 | 1   |
| C8660 | CONTROL SERUM Deamidated Gliadin-G | 879  | 2023-10 | 1   |

## CONTROLS


|  | Found results | Expected results |
|--|---------------|------------------|
|--|---------------|------------------|

|                       |       |            |
|-----------------------|-------|------------|
| Calibrator (mOD)      | 360   | $\geq 100$ |
| Control Serum (AU/mL) | 127,1 | 71,9-212,0 |

## CALIBRATOR

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 2 | 5 | 5 | 8 | 7 | 9 | 6 | 1 | 2 | 0 | 3 | 6 | 2 | 6 | 6 | 1 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader YES ☒ Operator Signature .....

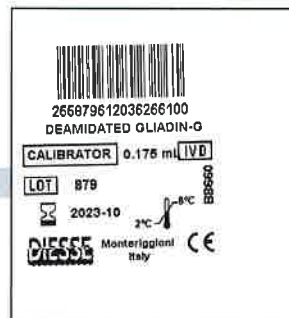

## CONTROL SERUM

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 2 | 5 | 5 | 8 | 7 | 9 | 6 | 2 | 7 | 5 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader YES ☒ Operator Signature .....

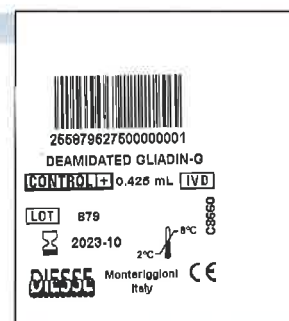

*This batch has been manufactured and checked according to quality requirements.  
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents.....

DATE .....

## WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.