

DIESSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

## QUALITY CONTROL CERTIFICATE

KIT NAME DEAMIDATED GLIADIN-G - CHORUS

|         |       |         |         |
|---------|-------|---------|---------|
| Code    | 86100 |         |         |
| Lot No. | 007   | 2025-02 | 2024-02 |

### REAGENTS

| Label | Description                        | Lot. | Exp.    | NO  |
|-------|------------------------------------|------|---------|-----|
| D8660 | Deamidated Gliadin-G               | 007  | 2025-02 | 6X6 |
| B8660 | CALIBRATORE Deamidated Gliadin-G   | 007  | 2025-02 | 1   |
| C8660 | CONTROL SERUM Deamidated Gliadin-G | 007  | 2025-02 | 1   |

### CONTROLS


|  | Found results | Expected results |
|--|---------------|------------------|
|--|---------------|------------------|

|                       |      |            |
|-----------------------|------|------------|
| Calibrator (mOD)      | 542  | $\geq 100$ |
| Control Serum (AU/mL) | 49,7 | 32,5-85,0  |

### CALIBRATOR

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 2 | 5 | 5 | 0 | 0 | 7 | 6 | 1 | 2 | 2 | 3 | 2 | 4 | 5 | 5 | 4 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader YES ☒ Operator Signature FB

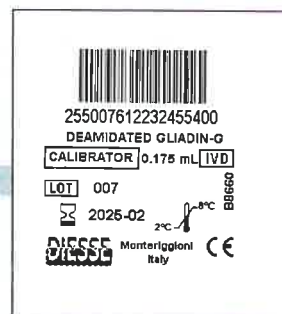

### CONTROL SERUM

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 2 | 5 | 5 | 0 | 0 | 7 | 6 | 1 | 6 | 2 | 9 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader YES ☒ Operator Signature FB

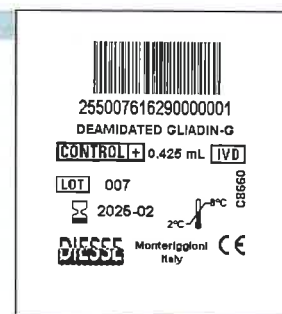

*This batch has been manufactured and checked according to quality requirements.  
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents FB

DATE 21/02/2024

### WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.