

DIESSE DIAGNOSTICA SENESE SpA
53035 Monteriggioni (SI) – Italia – Via delle Rose 10
Tel +39-0577-587111 Fax +39-0577-318690



Pag 1/1
Sede Legale e Amministrazione
20144 Milano (Italy) Via A. Solari 19 sc. 6
Tel. +39-02-4859121 r.a. Fax +39-02-48008530

QUALITY CONTROL CERTIFICATE

KIT NAME: CHORUS PHOSPHOLIPID SCREEN IgM

Code	86108		
Lot No.	860	2023-08	2022-08

REAGENTS

Label	Description	Lot.	Exp	No
D4020	Phospholipid Screen IgM	860	2023-08	6x6
B4020	CALIBRATORE Phospholipid Screen IgM	860	2023-08	1
C4020	CONTROL SERUM Phospholipid Screen IgM	860	2023-08	1

CONTROLS

Found results	Expected results
---------------	------------------

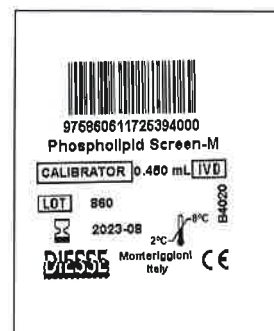
Calibrator (mOD)	490	≥ 100
Control (AU/ml)	45,1	22,5-61,3

CALIBRATOR

9	7	5	8	6	0	6	1	1	7	2	5	3	9	4	0	0	0
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader

YES

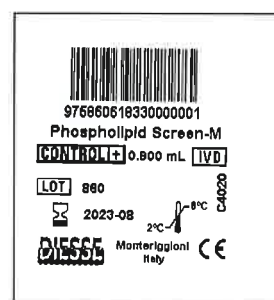
Operator Signature *SB*

CONTROL SERUM

9	7	5	8	6	0	6	1	8	3	3	0	0	0	0	0	0	1
---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---	---

Label checked with barcode reader

YES

Operator Signature *SB*

The test has been carried out in accordance with the package insert

TESTED BY: Sara Benocci *Benocci*APPROVED RESPONSIBLE HEAD, Quality Control Reagents *Alciandri*DATE *09.09.2022*

WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested by an FDA approved method and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.