

DIESSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

## QUALITY CONTROL CERTIFICATE

KIT NAME Epstein-Barr VCA IgM II - CHORUS

|         |       |         |         |
|---------|-------|---------|---------|
| Code    | 81054 |         |         |
| Lot No. | 926   | 2024-07 | 2023-04 |

## REAGENTS

| Label | Description                           | Lot. | Exp.    | NO  |
|-------|---------------------------------------|------|---------|-----|
| D9490 | Epstein-Barr VCA IgM II               | 926  | 2024-07 | 6x6 |
| B9490 | CALIBRATOR Epstein-Barr VCA IgM II    | 926  | 2024-07 | 1   |
| C9490 | CONTROL SERUM Epstein-Barr VCA IgM II | 926  | 2024-07 | 1   |

## CONTROLS


|  | Found results | Expected results |
|--|---------------|------------------|
|--|---------------|------------------|

|                          |     |            |
|--------------------------|-----|------------|
| Calibrator (mOD)         | 540 | $\geq 100$ |
| Control Serum (INDEX)    | 2,2 | 1,4-2,7    |
| Negative Control (INDEX) | 0,0 | $< 0,7$    |

## CALIBRATOR

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 0 | 3 | 0 | 9 | 2 | 6 | 7 | 0 | 0 | 0 | 0 | 0 | 4 | 9 | 0 | 0 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader YES ☒ Operator Signature

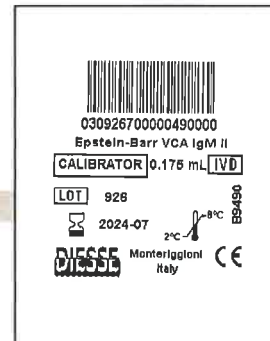

## CONTROL SERUM

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 0 | 3 | 0 | 9 | 2 | 6 | 7 | 1 | 4 | 2 | 7 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader YES ☒ Operator Signature

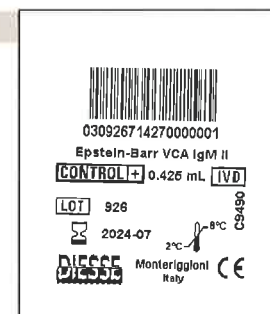

*This batch has been manufactured and checked according to quality requirements.  
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents.....

DATE 27.04.2023

## WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.