

DIESSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

### QUALITY CONTROL CERTIFICATE

KIT NAME CHLAMYDOPHILA PNEUMONIAE IgG - CHORUS

Code 81250

Lot No. 935



2024-05



2023-05

### REAGENTS

| Label | Description                         | Lot. | Exp.    | NO  |
|-------|-------------------------------------|------|---------|-----|
| D8590 | Chlamydomphila pneumoniae IgG       | 935  | 2024-05 | 6X6 |
| B8590 | CALIBRATORE Chlamydomphila p. IgG   | 935  | 2024-05 | 1   |
| C8590 | CONTROL SERUM Chlamydomphila p. IgG | 935  | 2024-05 | 1   |

### CONTROLS

|  | Found results | Expected results |
|--|---------------|------------------|
|--|---------------|------------------|

|                          |         |             |
|--------------------------|---------|-------------|
| Calibrator (mOD)         | 360     | $\geq 100$  |
| Control Serum (AU/mL)    | 53,8    | 30,8-95,7   |
| Negative Control (AU/mL) | $<10,0$ | $\leq 10,0$ |

### CALIBRATOR

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 2 | 2 | 2 | 9 | 3 | 5 | 6 | 6 | 1 | 5 | 2 | 8 | 3 | 2 | 4 | 2 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader

YES



Operator Signature .....

*RB*

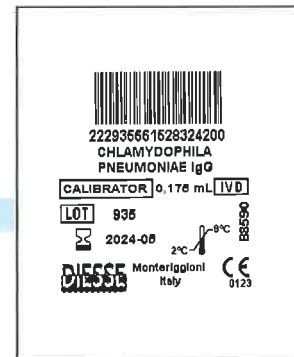

### CONTROL SERUM

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 2 | 2 | 2 | 9 | 3 | 5 | 6 | 2 | 2 | 4 | 1 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader

YES



Operator Signature .....

*RB*



*This batch has been manufactured and checked according to quality requirements.  
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents.....

*[Signature]*

DATE 18/05/2023

### WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.