

DIESSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

## QUALITY CONTROL CERTIFICATE

KIT NAME CHIKUNGUNYA IgM -CHORUS

|         |       |  |         |  |         |
|---------|-------|--|---------|--|---------|
| Code    | 81134 |  |         |  |         |
| Lot No. | 940   |  | 2024-05 |  | 2023-05 |

## REAGENTS

| Label | Description                 | Lot. | Exp.    | NO  |
|-------|-----------------------------|------|---------|-----|
| D0211 | CHIKUNGUNYA IgM             | 940  | 2024-05 | 6x6 |
| B0211 | CALIBRATORE CHIKUNGUNYA IgM | 940  | 2024-05 | 1   |
| C0211 | CONTROL CHIKUNGUNYA IgM     | 940  | 2024-05 | 1   |

## CONTROLS

|                  | Found results | Expected results |
|------------------|---------------|------------------|
| Calibrator (mOD) | 320           | $\geq 100$       |
| Control (INDEX)  | 1,8           | 1,4-2,6          |

## CALIBRATOR

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 9 | 1 | 0 | 9 | 4 | 0 | 6 | 0 | 0 | 0 | 0 | 0 | 5 | 1 | 0 | 0 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader YES ☒ Operator Signature



## CONTROL SERUM

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 9 | 1 | 0 | 9 | 4 | 0 | 6 | 1 | 4 | 2 | 6 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader YES ☒ Operator Signature

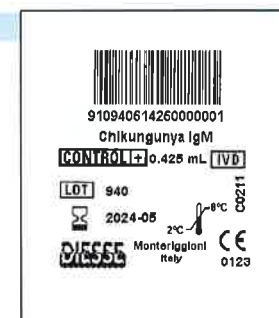

*This batch has been manufactured and checked according to quality requirements.  
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents

DATE 12/06/2023

## WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.