

DIESSE DIAGNOSTICA SENESE SpA  
53035 Monteriggioni (SI), Italy, Strada dei Laghi 39  
Tel. +39 0577319554 FAX +39 0577319020



Sede Legale  
20144 Milano (Italy) Via A. Solari 19 sc. 6

Pag 1/1

## QUALITY CONTROL CERTIFICATE

KIT NAME CHLAMYDOPHILA PNEUMONIAE IgA - CHORUS

Code 81252

Lot No. 954



2024-07



2023-07

### REAGENTS

| Label | Description                         | Lot. | Exp.    | NO  |
|-------|-------------------------------------|------|---------|-----|
| D8610 | Chlamydomphila pneumoniae IgA       | 954  | 2024-07 | 6X6 |
| B8610 | CALIBRATORE Chlamydomphila p. IgA   | 954  | 2024-07 | 1   |
| C8610 | CONTROL SERUM Chlamydomphila p. IgA | 954  | 2024-07 | 1   |

### CONTROLS


|  | Found results | Expected results |
|--|---------------|------------------|
|--|---------------|------------------|

|                          |       |             |
|--------------------------|-------|-------------|
| Calibrator (mOD)         | 525   | $\geq 100$  |
| Control Serum (AU/mL)    | 26,1  | 15,0-37,5   |
| Negative Control (AU/mL) | <10,0 | $\leq 10,0$ |

### CALIBRATOR

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 1 | 9 | 9 | 9 | 5 | 4 | 6 | 8 | 1 | 1 | 1 | 9 | 7 | 1 | 2 | 9 | 0 | 0 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|


Label checked with barcode reader YES ☒ Operator Signature *FB*

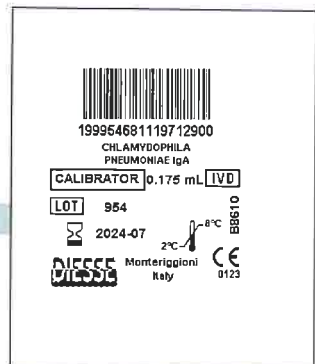

### CONTROL SERUM

|   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |   |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|
| 1 | 9 | 9 | 9 | 5 | 4 | 6 | 1 | 0 | 1 | 8 | 0 | 0 | 0 | 0 | 0 | 0 | 1 |
|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|---|

Label checked with barcode reader YES ☒ Operator Signature *FB*

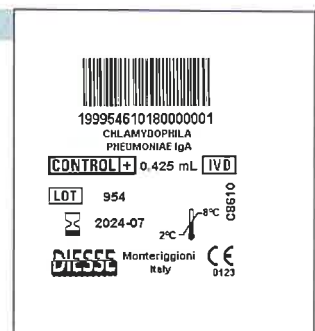

*This batch has been manufactured and checked according to quality requirements.  
Hereby, it is released to distribution.*

APPROVED RESPONSIBLE HEAD, Quality Control Reagents. *June*

DATE 26/09/2023

### WARNING: POTENTIAL BIOHAZARDOUS MATERIAL!

This kit may contain some reagents made with human serum or plasma. All serum or plasma used has been tested and found non-reactive for HIV-1/2, HCV and HBsAg. Because no method can offer complete assurance that HIV-1/2, HCV, HBsAg or other infectious agents are absent, reagents should be handled with maximum attention.